

APPLICATION

Extraction of 25-OH-Vitamin D2 and D3 from Serum by Novum™ Simplified Liquid Extraction (SLE) and LC/MS/MS Analysis using a Kinetex® 2.6µm F5 HPLC/UHPLC Column

Xianrong (Jenny) Wei and Matt Brusius
Phenomenex, Inc., 411 Madrid Ave., Torrance, CA 90501 USA

Overview

The aim of this application note is to introduce a fast and effective sample preparation technique using Novum Simplified Liquid Extraction (SLE) products that overcomes the challenges observed in a traditional liquid-liquid extraction (LLE). This rapid cleanup is then paired with an LC/MS/MS method using a Kinetex 2.6µm F5 core-shell HPLC column, resulting in >80% recoveries.

Sample Pre-treatment Step

To 200µL human serum spiked with 30µL 25-OH-Vitamin D3-d3 (1µg/mL in water) add 190µL of 2% Ammonium hydroxide in water and vortex for 30 seconds.

Extraction Procedure

Sample Loading

- Load the sample from pre-treatment step onto the Novum SLE 3 cc tube (Part No. 8B-S138-5BJ) and apply a short and gentle pulse of vacuum (~5-10 sec at 5" or less of Hg) until the sample has completely entered the media.
NOTE: Avoid prolonged or excessive vacuum. The sample must not leave the Novum bed.
- Wait for 5-6 minutes.
NOTE: Inadequate or excessive wait period will lead to variable recoveries and poor precision.

Elution

- Dispense 3x 600µL of ethyl acetate onto the Novum SLE sorbent and collect the solvent under force of gravity.
- Apply vacuum at 5" of Hg (or lower) for 20-30 secs to complete the extraction.

Dry Down

- Evaporate extracted samples to complete dryness under slow stream of N₂ and room temperature.
- Reconstitute the dry residue in 200µL of 0.1% Formic acid in Water/0.1% Formic acid in Methanol (30:70).

HPLC Conditions

Column: Kinetex 2.6µm F5
Dimensions: 100 x 4.6mm
Part No.: 00D-4723-E0
Mobile Phase: A: 0.1% Formic acid in Water
B: 0.1% Formic acid in Methanol
Gradient:

Time (min)	% B
0.00	85
5.00	85
5.01	100
6.50	100
6.51	85
8.00	85




Flow Rate: 0.75 mL/min
Temperature: Ambient
Detection: MS/MS, API 5000™ (AB SCIEX), APCI+
Injection: 10µL

Analyte	RT, min	Q1, Da	Q3, Da	CE
25-OH-Vitamin D2	4.16	395.3	209.3	30
		395.3	269.1	22
25-OH-Vitamin D3	3.93	383.6	257.2	25
		383.6	159.1	30
3-epi-25-OH-Vitamin D3	4.30	383.6	257.2	25
		383.6	159.1	30
25-OH-Vitamin D3-d3 (IS)	4.00	386.6	257.2	23
		386.6	368.4	20

Analyte Recovery

Analyte	% Absolute recovery (100 ng/mL)	%CV (N=6)
25-OH-Vitamin D2	80.4	5.03
25-OH-Vitamin D3	92.6	6.03
3-epi-25-OH-Vitamin D3	87.2	5.22

Representative Chromatograms

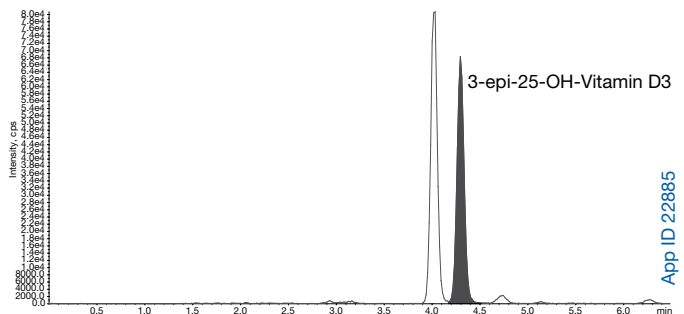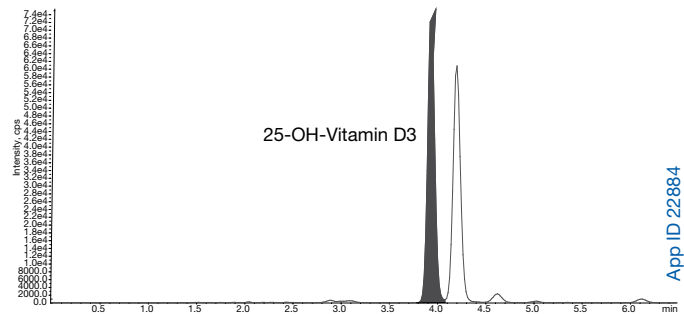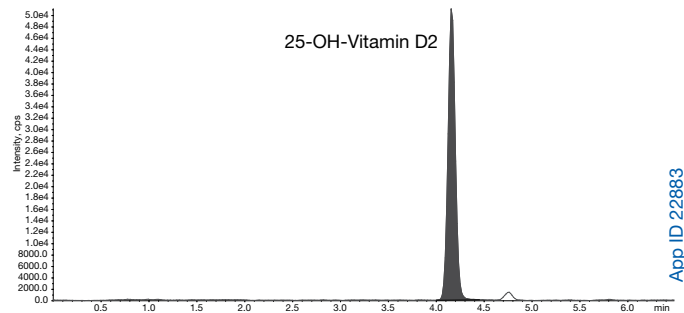

APPLICATION

Ordering Information

Novum™ Simplified Liquid Extraction (SLE)

96-Well Plates

Part No.	Description	Unit/Box
8E-S138-FGA	Novum SLE MINI 96-Well Plate	1/Box
8E-S138-5GA	Novum SLE MAX 96-Well Plate	1/Box

Tubes

Part No.	Description	Unit
8B-S138-FAK	Novum SLE 1 cc tubes	100/box
8B-S138-5BJ	Novum SLE 3 cc tubes	50/box
8B-S138-JCH	Novum SLE 6 cc tubes	30/box
8B-S138-KDG	Novum SLE 12 cc tubes	20/box

Kinetex® Core-Shell HPLC/UHPLC Columns

2.6 µm Minibore Columns (mm) SecurityGuard™ ULTRA Cartridges†

Phases	50 x 2.1	100 x 2.1	150 x 2.1	3/pk
F5	00B-4723-AN	00D-4723-AN	00F-4723-AN	AJO-9322 for 2.1 mm ID

2.6 µm MidBore™ Columns (mm) SecurityGuard™ ULTRA Cartridges†

Phases	50 x 3.0	100 x 3.0	150 x 3.0	3/pk
F5	00B-4723-Y0	00D-4723-Y0	00F-4723-Y0	AJO-9321 for 3.0 mm ID

2.6 µm Analytical Columns (mm) SecurityGuard™ ULTRA Cartridges†

Phases	50 x 4.6	100 x 4.6	150 x 4.6	3/pk
F5	00B-4723-E0	00D-4723-E0	00F-4723-E0	AJO-9320 for 4.6 mm ID

†SecurityGuard ULTRA Cartridges require holder, Part No.: AJO-9000

Australia
t: +61 (0)2-9428-6444
f: +61 (0)2-9428-6445
auiinfo@phenomenex.com

Austria
t: +43 (0)1-319-1301
f: +43 (0)1-319-1300
anfrage@phenomenex.com

Belgium
t: +32 (0)2 503 4015 (French)
t: +32 (0)2 511 8666 (Dutch)
f: +31 (0)30-2383749
beinfo@phenomenex.com

Canada
t: +1 (800) 543-3681
f: +1 (310) 328-7768
info@phenomenex.com

China
t: +86 (0)20 2282-6668
f: +86 (0)20 2809-8130
chinainfo@phenomenex.com

Denmark
t: +45 4824 8048
f: +45 4810 6265
nordicinfo@phenomenex.com

Finland
t: +358 (0)9 4789 0063
f: +45 4810 6265
nordicinfo@phenomenex.com

France
t: +33 (0)1 30 09 21 10
f: +33 (0)1 30 09 21 11
franceinfo@phenomenex.com

Germany
t: +49 (0)6021-58830-0
f: +49 (0)6021-58830-11
anfrage@phenomenex.com

India
t: +91 (0)40-3012 2400
f: +91 (0)40-3012 2411
indiainfo@phenomenex.com

Ireland
t: +353 (0)1 247 5405
f: +44 1625-501796
eirinfo@phenomenex.com

www.phenomenex.com

Phenomenex products are available worldwide. For the distributor in your country, contact Phenomenex USA, International Department at international@phenomenex.com

Italy
t: +39 051 6327511
f: +39 051 6327555
italiainfo@phenomenex.com

Luxembourg
t: +31 (0)30-2418700
f: +31 (0)30-2383749
nlinfo@phenomenex.com

Mexico
t: 001-800-844-5226
f: 001-310-328-7768
tecnicomx@phenomenex.com

The Netherlands
t: +31 (0)30-2418700
f: +31 (0)30-2383749
nlinfo@phenomenex.com

New Zealand
t: +64 (0)9-4780951
f: +64 (0)9-4780952
nzinfo@phenomenex.com

Norway
t: +47 810 02 005
f: +45 4810 6265
nordicinfo@phenomenex.com

Puerto Rico
t: +1 (800) 541-HPLC
f: +1 (310) 328-7768
info@phenomenex.com

Sweden
t: +46 (0)8 611 6950
f: +45 4810 6265
nordicinfo@phenomenex.com

United Kingdom
t: +44 (0)1625-501367
f: +44 (0)1625-501796
ukinfo@phenomenex.com

USA
t: +1 (310) 212-0555
f: +1 (310) 328-7768
info@phenomenex.com

**All other countries
Corporate Office USA** 
t: +1 (310) 212-0555
f: +1 (310) 328-7768
info@phenomenex.com



If Phenomenex products in this technical note do not provide at least equivalent separations as compared to other products of the same phase, size and dimensions, return the product with comparative data within 45 days for a FULL REFUND.

Terms and Conditions

Subject to Phenomenex Standard Terms and Conditions which may be viewed at www.phenomenex.com/TermsAndConditions.

Trademarks

Kinetex is a registered trademark and Novum, SecurityGuard, and MidBore are trademarks of Phenomenex. API 5000 is a trademark of AB SCIEX Pte. Ltd. AB SCIEX is being used under license.

Novum is patent pending.

Disclaimer

The products mentioned are not intended for clinical use. Because they are not intended for clinical use, no claim or representation is made or intended for their clinical use (including, but not limited to diagnostic, prognostic, therapeutic or blood banking). It is the user's responsibility to validate the performance of Phenomenex products for any particular use, since the performance characteristics are not established. Phenomenex products may be used in clinical diagnostic laboratory systems after the laboratory has validated their complete system as required by the Clinical Laboratory Improvements Amendments of 1988 (CLIA '88) regulation in the U.S. or equivalent in other countries.

© 2015 Phenomenex, Inc. All rights reserved.