

# APPLICATIONS

## Comparison of Antipsychotics Extracted from Human Plasma Using Microelution SPE

Shahana Huq<sup>1</sup> and Swetha Kotikalapudi<sup>2</sup>

<sup>1</sup>Phenomenex, Inc., 411 Madrid Ave, Torrance, CA 90501, USA

<sup>2</sup>Phenomenex, Ltd., Laxmi Cyber City, Ground Floor, B Block, Survey no: 10 Kondapur, Hyderabad 500 084, India

### Overview

This application describes a simple but effective sample preparation solution to increase productivity. Nine antipsychotics from human serum were extracted with ultra-sensitive Solid Phase Extraction (SPE) methods using Strata<sup>®</sup>-X-C Microelution 96-well plate and another product. While using a cation-exchange polymeric SPE sorbent packed in 96-well plate in microelution format, labs are able to skip the dry-down step saving at least 30 minutes without negatively impacting the sensitivity of their analysis. The small volume of biological samples loaded onto the ion-exchange sorbent, undergoes a 100% organic wash to result in a clean extract. The miniature elution volume capability of the packed 2 mg sorbent results in a 4x concentration enrichment of the nine basic antipsychotic drugs tested. This pre-concentration feature bypasses the need for dry down and reconstitution of the extracted samples before injection onto the LC-MS/MS. Possibility of analyte loss during dry-down is also eliminated for heat labile drugs. The reduction of sample processing time in a microelution format speeds up laboratory workflow by at least 50%.

The nine antipsychotics were accurately quantified by LC-MS/MS using a Kinetex<sup>®</sup> 2.6 μm PS C18 LC column. Kinetex has core-shell particle morphology that provides ultra-high column efficiency on any HPLC or UHPLC. The Kinetex PS C18 is a USP classified L1 column, that provides both a unique polar and hydrophobic selectivity and is 100% aqueous stable.

### Materials and Methods

Analytical reference standards and internal standards were purchased from Cerilliant Corporation (Round Rock, TX, USA). Human plasma was obtained from BioreclamationIVT (Westbury, NY). All other reagents and chemicals were purchased from Sigma-Aldrich (St. Louis, MO). Ultrapure D.I. water was obtained from Sartorius arium comfort II, courtesy of Sartorius Corporation (Bohemia, NY).

### SPE Protocol


<b>96-Well Microelution Plate:</b>	Strata-X-C Microelution Plate, 2 mg/well Brand A Plate, 2 mg/well
<b>Part No.:</b>	<a href="#">8M-S029-4GA</a> (for Strata-X-C)
<b>Condition:</b>	200 μL Methanol
<b>Equilibrate:</b>	200 μL Water
<b>Load:</b>	400 μL diluted human plasma (200 μL plasma diluted 1:1 with 4% Phosphoric acid in Water)
<b>Wash 1:</b>	200 μL 2% Formic acid in Water
<b>Wash 2:</b>	200 μL Methanol
<b>Elute:</b>	2x 25 μL 5% Ammonium hydroxide in Acetonitrile/Methanol (60:40)
<b>Spike IS:</b>	Spike 50 μL of internal standard in Methanol/Water (50:50) Sample was directly injected onto LC-MS/MS

### LC Conditions


<b>Column:</b>	Kinetex 2.6 μm PS C18	
<b>Dimension:</b>	50 x 2.1 mm	
<b>Part No.:</b>	<a href="#">00B-4780-AN</a>	
<b>SecurityGuard™ ULTRA:</b>	<a href="#">AJ0-8951</a>	
<b>Mobile Phase:</b>	A: 0.1% Formic acid in Water B: 0.1% Formic acid in Methanol	
<b>Gradient:</b>	<b>Time (min)</b>	<b>% B</b>
	0	5
	3	95
	3.5	95
	3.51	5
	5	5
<b>Flow Rate:</b>	0.5 mL/min	
<b>Injection Volume:</b>	2 μL	
<b>Temperature:</b>	Ambient	
<b>LC Instrument:</b>	Agilent 1260	
<b>Detector:</b>	SCIEX® Triple Quad™ 4500 (ESI, +ve Ionization)	

**Results and Discussions**

**Figure 1.** Representative Chromatogram of Extracted Plasma Sample Using Strata®-X-C 96-Well Microelution Plate

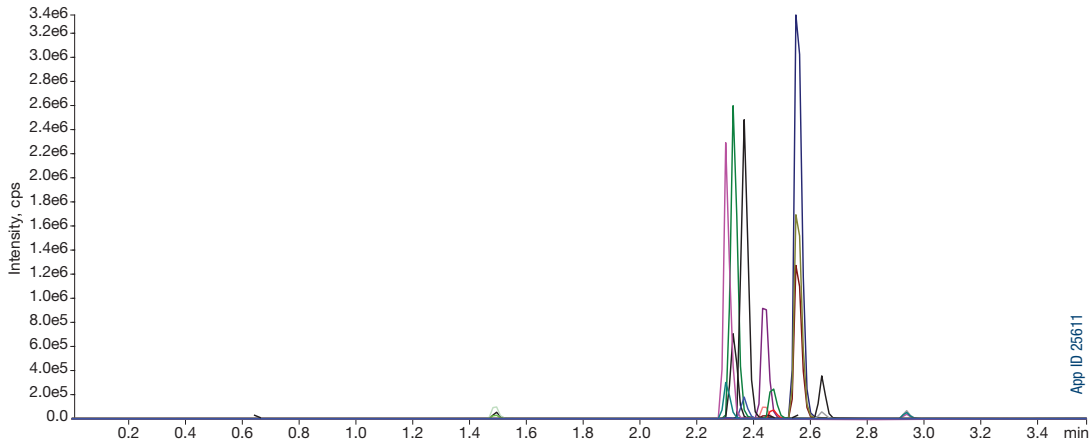

**Figure 2.** Representative Chromatogram of Extracted Plasma Sample Using Brand A Plate

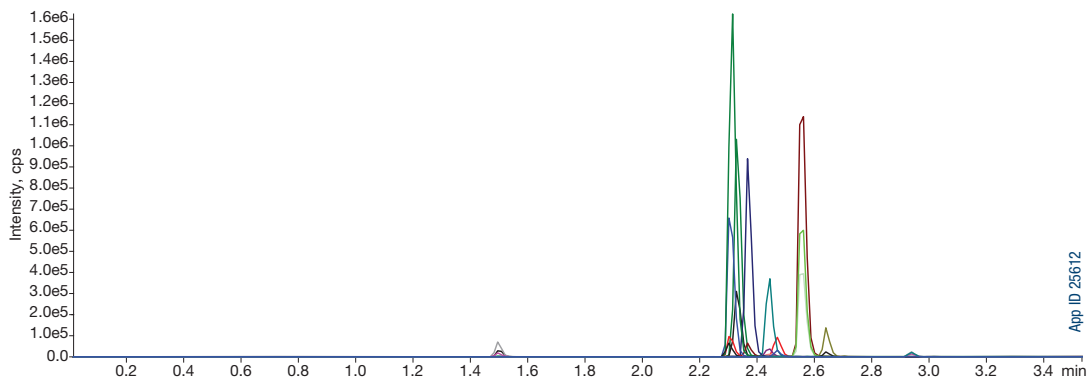

**Table 1.** % Absolute Recovery and CV for Extracted Plasma Samples

Antipsychotics	Spiked conc. (ng/mL)	RT (min)	Strata-X-C Microelution		Brand A	
			% Recovery	% CV (N=4)	% Recovery	% CV (N=4)
9-OH Risperidone	25	2.33	90	6.6	97	7.9
Olanzapine	25	1.53	98	6.9	101	8.6
Clozapine	25	2.47	95	4.0	98	6.6
Quetiapine	25	2.58	91	2.7	95	5.2
Norquetiapine	25	2.5	71	5.5	70	5.9
Risperidone	25	2.39	98	6.0	111	4.1
Norclozapine	25	2.36	92	7	106	12
Ziprasidone	25	2.67	61	10.7	68	6.8
Aripiprazole	25	2.96	65	6.0	79	0.7

Comparative separations may not be representative of all applications.


The recommended LC conditions for the Kinetex® PS C18 LC column efficiently and sensitively resolved nine antipsychotics, which are basic in nature and closely related in chemical properties. The recovery values for Strata®-X-C averaged about 85 % and 92 % for Brand A respectively, with the % recovery for each analyte seen in **Table 1**. Strata-X-C displays predominantly consistent results with lower %CVs for more analytes compared to Brand A. The parallel study of the above two cation-exchange sorbent shows very minor differences in recovery while microelution format was utilized. When observing **Figure 1 and 2** sensitivities can be compared of the two microelution formats being used with a Kinetex PS-C18 LC column showing the separation.

### Conclusions


In a laboratory workflow, at least 50 % of the total time spent in preparing and processing samples are from dry-down and reconstitution. The microelution format of the SPE increases the productivity of the sample prep process by eliminating the prolonged solvent evaporation and reconstitution, leaving it more simple and efficient. Our study under equal and controlled conditions demonstrated equivalent results for Phenomenex's Strata-X-C and another brand products in microelution format. The Kinetex PS C18 HPLC/UHPLC column's unique multi-modal selectivity and improved chromatographic performance when applied to the analysis of polar basic compounds. The unique selectivity and performance benefits of the Kinetex PS C18 were compared across certain antipsychotics to confirm consistent peak performance and selectivity.

### Ordering Information


#### Strata-X-C

Format	Sorbent Mass	Part Number	Unit
Tube			
	30 mg	<a href="#">8B-S029-TAK**</a>	1 mL (100/box)
	30 mg	<a href="#">8B-S029-TBJ</a>	3 mL (50/box)
	60 mg	<a href="#">8B-S029-UBJ**</a>	3 mL (50/box)
	100 mg	<a href="#">8B-S029-EBJ</a>	3 mL (50/box)
	100 mg	<a href="#">8B-S029-ECH</a>	6 mL (30/box)
	200 mg	<a href="#">8B-S029-FBJ</a>	3 mL (50/box)
	200 mg	<a href="#">8B-S029-FCH</a>	6 mL (30/box)
	500 mg	<a href="#">8B-S029-HBJ</a>	3 mL (50/box)
	500 mg	<a href="#">8B-S029-HCH</a>	6 mL (30/box)

#### 96-Well Plate

	10 mg	<a href="#">8E-S029-AGB</a>	2 Plates/Box
	30 mg	<a href="#">8E-S029-TGB</a>	2 Plates/Box
	60 mg	<a href="#">8E-S029-UGB</a>	2 Plates/Box

#### 96-Well Microelution Plate

	2 mg	<a href="#">8M-S029-4GA</a>	ea
--	------	-----------------------------	----

More part numbers available online.  
\*\*Tab-less tubes available.

### On-line Extraction Cartridge

Description	Part Number	Unit/Box
Strata-X-C on-line extraction cartridge, 20 x 2.0 mm	<a href="#">00M-S048-B0-CB</a>	ea
Cartridge holder, 20 mm	<a href="#">CHO-5845</a>	ea

### Kinetex Core-Shell LC Columns

More part numbers available online.

2.6 µm Minibore Columns (mm)					SecurityGuard™ ULTRA Cartridges†
Phases	30 x 2.1	50 x 2.1	100 x 2.1	150 x 2.1	3/pk
PS C18	<a href="#">00A-4780-AN</a>	<a href="#">00B-4780-AN</a>	<a href="#">00D-4780-AN</a>	<a href="#">00F-4780-AN</a>	<a href="#">AJ0-8951</a>

for 2.1 mm ID

2.6 µm MidBore™ Columns (mm)					SecurityGuard ULTRA Cartridges†
Phases	50 x 3.0	100 x 3.0	150 x 3.0		3/pk
PS C18	<a href="#">00B-4780-Y0</a>	<a href="#">00D-4780-Y0</a>	<a href="#">00F-4780-Y0</a>		<a href="#">AJ0-8950</a>

for 3.0 mm ID

2.6 µm Analytical Columns (mm)					SecurityGuard ULTRA Cartridges†
Phases	50 x 4.6	100 x 4.6	150 x 4.6	250 x 4.6	3/pk
PS C18	<a href="#">00B-4780-E0</a>	<a href="#">00D-4780-E0</a>	<a href="#">00F-4780-E0</a>	<a href="#">00G-4780-E0</a>	<a href="#">AJ0-8949</a>

for 4.6 mm ID

† SecurityGuard ULTRA Cartridges require holder, Part No.: [AJ0-9000](#).



# APPLICATIONS

**Australia**

t: +61 (0)2-9428-6444  
 auinfo@phenomenex.com

**Austria**

t: +43 (0)1-319-1301  
 anfrage@phenomenex.com

**Belgium**

t: +32 (0)2 503 4015 (French)  
 t: +32 (0)2 511 8666 (Dutch)  
 beinfo@phenomenex.com

**Canada**

t: +1 (800) 543-3681  
 info@phenomenex.com

**China**

t: +86 400-606-8099  
 cninfo@phenomenex.com

**Denmark**

t: +45 4824 8048  
 nordicinfo@phenomenex.com

**Finland**

t: +358 (0)9 4789 0063  
 nordicinfo@phenomenex.com

**France**

t: +33 (0)1 30 09 21 10  
 franceinfo@phenomenex.com

**Germany**

t: +49 (0)6021-58830-0  
 anfrage@phenomenex.com

**India**

t: +91 (0)40-3012 2400  
 indiainfo@phenomenex.com

**Ireland**

t: +353 (0)1 247 5405  
 eireinfo@phenomenex.com

**Italy**

t: +39 051 6327511  
 italiainfo@phenomenex.com

**Luxembourg**

t: +31 (0)30-2418700  
 nlinfo@phenomenex.com

**Mexico**

t: 01-800-844-5226  
 tecnicomx@phenomenex.com

**The Netherlands**

t: +31 (0)30-2418700  
 nlinfo@phenomenex.com

**New Zealand**

t: +64 (0)9-4780951  
 nzinfo@phenomenex.com

**Norway**

t: +47 810 02 005  
 nordicinfo@phenomenex.com

**Poland**

t: 0-0-800-4911952  
 pl-info@phenomenex.com

**Portugal**

t: +351 221 450 488  
 ptinfo@phenomenex.com

**Singapore**

t: +65 800-852-3944  
 sginfo@phenomenex.com

**Spain**

t: +34 91-413-8613  
 espinfo@phenomenex.com

**Sweden**

t: +46 (0)8 611 6950  
 nordicinfo@phenomenex.com

**Switzerland**

t: +41 (0)61 692 20 20  
 swissinfo@phenomenex.com

**United Kingdom**

t: +44 (0)1625-501367  
 ukinfo@phenomenex.com

**USA**

t: +1 (310) 212-0555  
 info@phenomenex.com

🌐 **All other countries/regions  
 Corporate Office USA**

t: +1 (310) 212-0555  
 info@phenomenex.com

**www.phenomenex.com**

Phenomenex products are available worldwide. For the distributor in your country/region, contact Phenomenex USA, International Department at international@phenomenex.com

**Terms and Conditions**

Subject to Phenomenex Standard Terms & Conditions, which may be viewed at [www.phenomenex.com/TermsAndConditions](http://www.phenomenex.com/TermsAndConditions).

**Trademarks**

Strata and Kinetex are registered trademarks and SecurityGuard, MidBore, and Be-Happy are trademarks of Phenomenex. SCIEX is a registered trademark and Triple Quad is a trademark of AB SCIEX Pte. Ltd. AB SCIEX<sup>SM</sup> is being used under license. Sartorius and arium are registered trademarks of Sartorius AG.

**Disclaimer**

Comparative separations may not be representative of all applications. All data comparison information is for reference only in this catalog and is not intended to be used for comparison between different brands.

FOR RESEARCH USE ONLY. Not for use in clinical diagnostic procedures.

© 2020 Phenomenex, Inc. All rights reserved.